

xylem



Digital Refractometers & Polarimeters

FOR PRECISE MEASUREMENT OF CONCENTRATION AND PURITY



a xylem brand


Precision measurement of concentration and purity in laboratory or factory environments

What is Refractive Index?

When light passes from one medium to another, the speed at which the light travels will change depending on the parameters of the materials. This principle can be seen when looking at a straw in a glass or an oarsman on the river, as shown in the diagram.

The ratio or change in the speed of light is called refractive index and instruments that measure this are called refractometers.


The refractive index of a liquid is related to its concentration and so a refractometer can display the concentration in suitable units, such as °Brix (sucrose), glucose, sodium chloride, urea and urine specific gravity to name just a few.

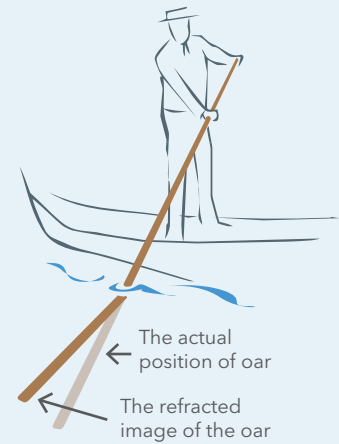

What is Optical Rotation?

When plane-polarised light passes through an optically active substance, the plane of polarisation will rotate by an amount that is specifically related to the product through which it travelled.

As many chemical compounds display this chiral characteristic, the measurement of optical rotation using a polarimeter is commonplace within the sugar, food, chemical and pharmaceutical manufacturing industries as a production control and quality assurance tool.

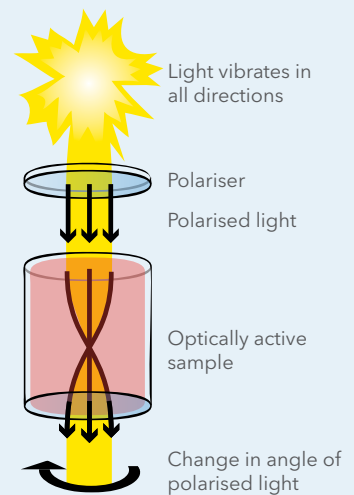

Feature Key



21 CFR Part 11



Peltier Temperature Control



RFID User Identity



Factory Friendly



USB Connectivity



HD Colour Display



All instruments shown in this brochure are made in the UK, except ADP600 series, made in USA.

RFM700 Refractometers



RFM700 series refractometers are robust, low cost, fully automatic instruments that are ideally suited to the food, sugar and beverage industries but can also be used in many other non-food applications where temperature control is not required.

Commonly, the RFM700-M series refractometers are supplied to operate in the °Brix scale with results temperature compensated to 20°C in accordance with ICUMSA. Additional user scales provide measurement in different formats such as Refractive Index (RI) various wine, urine specific gravity & automotive scales as well as allowing custom scales to be loaded in accordance with product data.

Inherent to the robust design is a sapphire prism mounted in an easy-clean stainless steel dish and an outer casing that is sealed and shaped to withstand sample spillage and moisture ingress. This, together with the external power supply and bright 4" high definition full colour display, makes the RFM700-M ideal for use in busy laboratories or harsh factory environments. The instrument can also save and/or print results and be connected to a printer or laboratory PC, with results being output in standard print, CSV or secure PDF formats.

Other software features include special AG temperature compensation that facilitates a SPAN calibration when using AG calibration fluids, and a time delay before reading, ensuring reliable results every time.



- Classic red or modern colour display
- Multiple scale
- Alphanumeric keypad
- Audit trail (date, time, batch & operator)
- USB connectivity

| Specifications | RFM712-M | RFM732-M | RFM742-M |
|----------------------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|----------------|------------------|
| Order Code | 19-00 | 19-10 | 19-20 |
| Scales | | | |
| °Brix | 0 - 50 | 0 - 100 | 0 - 100 |
| User Defined (RI equivalent) | 2 (1.33-1.42) | 2 (1.33-1.54) | 2 (1.33-1.54) |
| Resolution (°Brix/RI equivalent) | 0.1 (0,0001) | 0.1 (0.0001) | 0.01 (0.00001) |
| Accuracy (°Brix/RI equivalent) | ±0.1 (±0.0001) | ±0.1 (±0,0001) | ±0.04 (±0.00005) |
| Precision (Reproducibility) | | | |
| Refractive Index | ± 0.00005 | ± 0.00005 | ± 0.00001 |
| Sugar (°Brix) | ± 0.05 | ± 0.05 | ± 0.01 |
| Other Scales | 20+ pre-programmed scales including HFCS (3), Sugar (4), Honey, NaCl, Wine Must (5), Urine SG (3), Glycol (2), Urea, FSII and more; plus customer programmable user scales via PC. | | |
| Temperature Range | 5-40°C | | |
| Temperature Compensation | ICUMSA, AG, None or User Defined | | |
| Temperature Control | None - Temperature Compensation (ATC) | | |
| Temperature Sensor Accuracy | ±0.05°C | | |
| Temperature Stability Checks | Delay time (programmable in seconds) | | |
| Interface | 3 x USB (A), 1 x USB (B), Ethernet. RS232 via optional adaptor | | |

RFM300 Refractometers

The RFM300 Series of refractometers are the result of a combination of over 100 years' experience in design and manufacturing led by customer needs. With a wide measuring range and Peltier temperature control of the flat, easy clean prism, the RFM300 Series refractometers offer extremely rapid temperature stabilization of the sample, allowing readings to be taken quickly and reliably in any scale including Brix, Refractive Index (RI) or up to 100 user defined scales.



Whether a high resolution 7" touchscreen (RFM300-T) or a more tactile keypad (RFM300-M) is required, the graphical user interface with easy to use menus gives the RFM300 Series instruments a fresh, modern look and feel.

A large sampling area on the prism surface allows measurement of not only homogenous fluids like juices, sodas, sauces and edible oils, but also difficult to read samples like fruit pulps and industrial resins.

Intelligent software ensures rapid temperature response to changes in prism temperature, whilst the SMART temperature stability check makes sure that the result is displayed only when the sample is stable. A Methods system allows rapid configuration of instrument setup and provides limit checks against stored data as well as product-specific corrections, such as citric acid content for orange juice or coffee solids daily offsets. Over 8000 readings may be stored within the instrument memory and the on-screen menu may be displayed in a number of different languages.

The instrument is available in two formats, the most popular being the 3-decimal place Brix RFM340 refractometer, which, following improvements to the thermodynamic control system, now has an increased measurement performance between 0-30 °Brix and so reduces potential measurement error in the critical range covering finished products like the aforementioned juices and sodas. By improving the performance at the low end of the scale, users may now trim syrup dilution to the absolute minimum without the risk of breaching manufacturing specifications.

SG scales for sucrose are also common to the series. These scales may be used to express the relative density of pure sucrose solutions and, when used in conjunction with a product offset from within the Methods system, can express finished beverages as an equivalent SG. By doing so, contract packers of beverage products

- Touchscreen or keypad
- Easy clean prism
- High accuracy ($\pm 0.01^\circ$ Brix)
- Dual scale display
- Smart temperature stability
- Print to secure PDF

| RFM340+ | | Bellingham + Stanley a xylem brand | |
|----------------------------|--------------------------------------|---------------------------------------|----------------------|
| Device Information | | | |
| Serial Number: | RU12147 | Application SW: | 22.481.03 Rev. 0.106 |
| Calibration Details | | | |
| Last Zero: | 25/03/14 14:41, 1.33259 22.5 (pl no) | | |
| Last Span: | 19/03/14 14:49, 1.42009 22.5 (pl no) | | |
| Configuration | | | |
| Scale: | brix (brix) | TC: | sugar (suc) |
| Sol Temp: | 22.5°C | Resolution: | medium |
| Stability: | none | | |
| Lang: | none | | |
| Measurement Details | | | |
| Time / Date | Reading | Temperature | Quality |
| 12:21:25 26/03/14 | 30.34 | 22.5°C | 101 |
| 12:21:31 26/03/14 | 30.35 | 22.5°C | 100 |
| 12:21:35 26/03/14 | 30.34 | 22.5°C | 101 |
| 12:21:40 26/03/14 | 30.35 | 22.5°C | 100 |
| 12:21:44 26/03/14 | 30.35 | 22.5°C | 100 |
| 12:21:48 26/03/14 | 30.35 | 22.5°C | 100 |
| 12:21:53 26/03/14 | 30.35 | 22.5°C | 100 |
| 12:21:57 26/03/14 | 30.33 | 22.5°C | 100 |
| 12:22:01 26/03/14 | 30.33 | 22.5°C | 100 |
| 12:22:06 26/03/14 | 30.35 | 22.5°C | 100 |
| Mean: | 30.34 | 22.5 | |
| Std. dev.: | 0.006 | 0.06 | |
| Min: | 30.33 | 22.5 | |
| Max: | 30.35 | 22.5 | |
| Spread: | 0.02 | 0.0 | |
| 26/03/14 | | RU12147_140320_122125.pdf | |

may now use a refractometer in situations where density °Brix or SG is dictated as the method of analysis, whilst retaining all the measurement advantages held by a refractometer. A dual display function allows original Brix or RI to be displayed alongside the equivalent sucrose SG result.



Other new features now standard on the RFM300 Series include RFID User Clearance, electronic signatures and audit trails that facilitate use in an FDA regulated environment (21 CFR part 11) as well as enhanced functionality via the new USB interfaces such as Back-up & Clone and Print to Secure PDF.

| Specifications | RFM330 | RFM340 | RFM340 Refractometer Enhanced Performance | | |
|------------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|-------------------------------|----------------------------------------------|------------------|----------------------|
| | | | RFM340 | RI | °Brix |
| Order Code | | | Scale | 1.32-1.58 | 0-100 |
| RFM300-T | 19-30 | 19-40 | | 1) 1.32-1.38 | 1) 0-30 |
| RFM300-T | 19-35 | 19-45 | | 2) 1.38-1.58 | 2) 30-100 |
| Scales | | | Resolution | 0.000001 (6 d.p) | 0.001 (3 d.p) |
| Refractive Index | 1.32 - 1.58 | 1.32 - 1.58 | Precision | 0.000005 (6 d.p) | 0.005 (3 d.p) |
| Sugar (°Brix) | 0 - 100 | 0 - 100 | | | |
| User Defined | 100 | 100 | | | |
| Resolution | | | | | |
| Refractive Index | 0.00001 | 0.00001 | | | |
| Sugar (°Brix) | 0.01 | 0.01 | | | |
| Accuracy | | | | | |
| Refractive Index | ± 0.00005 | ± 0.00002 (1.32 - 1.38 RI) | | | |
| | | ± 0.00004 (1.38 - 1.58 RI) | | | |
| Sugar (°Brix) | ± 0.04 | ±0.01 (0 - 30 °Brix) | | | |
| | | ±0.03 (30 - 100 °Brix) | | | |
| User Scale Library on-board | 20+ preprogrammed scales including HFCS (3), wine (5), sugar (4), urine SG (3), Urea, sucrose SG (3), FSII, NaCl, Butyro etc. Plus customer programmable scales via PC. | | | | |
| Presser Type | Polyacetal | | | | |
| Reading Time | Minimum 4 seconds | | | | |
| Measuring Temperature Range | 0 °C or 10°C below ambient whichever is greater to 70 °C | | | | |
| Temperature Sensor Accuracy | ± 0.03°C | | | | |
| Sample Temperature Stability | ± 0.05°C | | | | |
| Temperature Compensation | | | | | |
| Sucrose (°Brix) | 5 - 70 °C | | | | |
| AG Fluids | 5 - 40 °C | | | | |
| User Defined | Simple coefficient (units/°C) or polynomial function | | | | |
| Temperature Stability Checks | None/delay time/repeatability/ Smart (independently selectable by Method) | | | | |
| Interfaces | 3 x USB (A), 1 x USB (B), Ethernet. RS232 via optional adaptor | | | | |
| Prism Seal | Silicon/Resin | | | | |



RFM900-T Refractometers

Featuring a new touchscreen display and wide measuring range up to 1.70 RI and capable of measuring to six decimal places, the RFM900-T Series refractometers are ideally suited for use in the chemical, petrochemical, pharmaceutical, flavours and fragrance industries as well as for academic research. The RFM900-T series of refractometers combine the latest opto-electronic principles with durability and ease of use. RFM900-T refractometers feature RFID (Radio Frequency Identification) that allows users to identify themselves by simply swiping a tag across the top of the instrument to enable measurement and, in certain cases, access to the configuration menu.

A low-profile sample dish and non-contact presser makes sample application and cleaning easy. Readings can be taken automatically on the replacement of the presser, and over 8000 stored results can be easily viewed in tabular form on the instrument display. Peltier temperature control and intelligent temperature management ensures readings are only taken when the sample and refractometer temperatures are both stable.

| Specifications | RFM960-T | RFM970-T | RFM990-AUS32 |
|------------------------------|---------------------------------------------------------------------------|---------------------|------------------------------------------------|
| Order Code | 19-60 | 19-70 | 19-73 |
| Scales | | | |
| Refractive Index | 1.30 - 1.70 | 1.30 - 1.70 | 1.30 - 1.70 |
| Sugar (°Brix) | 0 - 100 | 0 - 100 | 0 - 100 |
| User Defined | 100 | 100 | 0 - 40% Urea |
| Resolution | | | |
| Refractive Index | 0.0001 | 0.000001 | 0.000001 |
| Sugar (°Brix) | 0.1 | 0.001 | 0.001 |
| Accuracy | | | |
| Refractive Index | ± 0.0001 | ± 0.00002 | ± 0.00002 |
| Sugar (°Brix) | ± 0.1 | ± 0.02 | ± 0.02 |
| Precision | | | |
| Refractive Index | ± 0.00005 | ± 0.000005 (6 d.p.) | ± 0.000005 (6 d.p.) |
| Sugar (°Brix) | ± 0.05 | ± 0.005 | ± 0.005 |
| Presser Type | Polyacetal | Polyacetal | Polyacetal |
| Temperature Compensation | | | Urea, ICUMSA (sugar), AG, None or User Defined |
| Sucrose (Brix°) | | | |
| AG Fluids | 5 - 80 °C | | |
| User Defined | 5 - 40 °C | | |
| | Simple coefficient (units/°C) or polynomial function | | |
| Temperature Control | Peltier | | |
| Temperature Stability Checks | None/delay time/repeatability/ Smart (independently selectable by Method) | | |
| Measuring Temperature Range | 0°C or 10°C below ambient whichever is the greater to 80°C | | |
| Temperature Sensor Accuracy | ± 0.03°C | | ±0.02 °C (a 20°C) |
| Sample Temperature Stability | ± 0.02°C | | ±0.01 °C (a 20°C) |
| Prism Seal | FDA and Class VI approved | | |
| Interfaces | 3 x USB (A), 1 x USB (B), Ethernet. RS232 via optional adaptor | | |

The instruments conform to a number of industry measurement standards and offer operational features that allow use in an environment controlled by FDA regulation 21 CFR Part 11.

The use of a Kalrez® gasket and sapphire prism facilitates placement in the harshest measurement environments including those in the pharmaceutical, petrochemical, aroma, flavour, fragrance and other high RI sectors.



- Pharmaceutical
- Chemical
- Widest RI range
- Highest precision (± 0.000005 RI)
- MEAN Method (USP/EP/BP)
- All RFM900s conform to ASTM D 1218, 1747, 2140 & 5006
- FDA approved materials for wetted components
- Materials traceability Certificate available

RFM990-AUS32 Refractometer

The RFM990-AUS32 is an extremely high accuracy refractometer specifically designed to meet the stringent needs of the chemical manufacturing industry. Of particular interest is its compliance with the strictest of ISO procedures in relation to the manufacture of urea-based NOx reduction agents used as Diesel Exhaust Fluids, also known as DEF, AUS32 and AdBlue®.

ISO 22241 dictates the highest level of measurement must be achieved under the tightest limits of temperature control. In addition to the compliance with this norm, the RFM990-AUS32 is fitted with specific Urea scales and temperature compensation as well as an AUS32 Method that allows input of both the F factor and biuret content of the solution that is included in the analysis.

Being part of the RFM900 series of refractometers, users of the RFM990-AUS32 also benefit from common features such as RFID user identity/clearance, on-board data storage, limit checking and audit trails.

No matter how good the instrument performance, without good verification it is not possible to confirm the instrument meets the specification laid down in ISO 22241. Bellingham + Stanley offer a UKAS Certified Reference Material for this purpose at the equivalent RI value of Urea stated in the norm.



- Petrochemical model
- Premium performance
- Conforms to ISO 22241
- AUS32 Method (input criteria)

AdBlue® is a registered trademark of the VDA Verband der Automobilindustrie e.V.
Kalrez® is a registered trademark of DuPont Performance Elastomers LLC.
1. AUS32 performance - 20°C is mandatory.

Common Specifications - Laboratory Refractometers

| | |
|---------------------|---------------------------------------------------------------------------------------------------------|
| Prism | Artificial Sapphire (1.76RI - Hardness 9.0 Mohs) |
| Prism Dish | 316 Stainless Steel with PEEK spill barrier |
| Sample Illumination | Light Emitting Diode 589nm (100,000+ hours) |
| Reading Time | Minimum 4 seconds (stability checks on all models) |
| Instrument Housing | Acrylonitrile Butadiene Styrene (ABS) |
| Power | Instrument: 24 V DC, $\pm 5\%$, <2A Power Supply Unit: 100-240V, 50-60Hz (supplied with instrument) |
| Humidity Range | <90% RH (non condensing) |

ADP400 Polarimeters



The ADP400 Series of general-purpose, single wavelength polarimeters are suitable for sugar, food, chemical and pharmaceutical industries where measurement is required to 3-decimal place resolution ($^{\circ}\text{A}$) over a length between 10 and 200mm. The ADP400 polarimeters are available with or without XPC - Xylem's patented internal Peltier temperature control system.




ADP400 series polarimeters feature a 'no maintenance' LED light source and interference filter with photodiode detector technology that provides sample readings up to 3.0 OD at the commonly used sodium (589nm) wavelength. Conveniently, ADP400 Series instruments use standard polarimeter tubes or for scarce samples, low volume luer taper tubes.

ADP400 Series polarimeters now feature a full colour, 4" (10 cm) high definition display. Measurement may be expressed as angular degrees ($^{\circ}\text{A}$), sugar (ISS) or user programmable scales, with standard Methods facilitating display of invert sugar,

| Specifications | Angular ($^{\circ}\text{A}$) | ISS ($^{\circ}\text{Z}$) |
|------------------------------|--------------------------------|----------------------------|
| Scales | -355 a +355 (selectable) | -225 à +225 |
| Resolution | 0.01/0.001 | 0.01/0.001 |
| Accuracy | ± 0.010 | ± 0.030 |
| Precision (Reproducibility)* | ± 0.002 | ± 0.005 |


Common Specifications - Laboratory Polarimeters & Saccharimeters (ADP/S 400 Series)

| | |
|------------------------|----------------------------------------------------------------------------------------------|
| Sample Illumination | Light Emitting Diode (100,000 hrs). Interference Filter 589nm (except ADS480: 850nm) |
| Beam Diameter | 4 mm |
| Optical Path Length | 10 to 200 mm |
| Optical Density Range | 0.0 to 3.0 OD (except ADS480) |
| Reading Type | Selectable continuous measurement or single shot (ADP) or continuous (ADS) |
| Reading Time (seconds) | 4-30 selectable by Method (AD) or 20 (ADS) |
| Instrument Housing | Polyurethane foam with aluminium base |
| Power | Instrument: 24 V DC, $\pm 5\%$, $< 2\text{A}$ External PSU: 100-240V, 50-60Hz (supplied) |
| Humidity Range | $< 90\%$ RH (non condensing) |
| Interfaces | 1 x USB (A), 1 x USB (B), 1 x Ethernet |
| Data Output | Print to USB, print to printer, csv, XML |

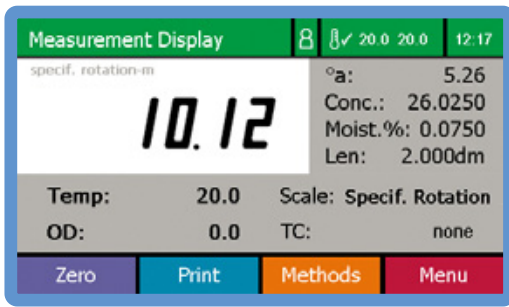


inversion (A-B) or, when applying other factors such as tube length and concentration, Specific Rotation (or concentration when entering specific rotation).

The ADP400 Series offers both continuous and 'single-shot' reading modes, the latter being ideal for pharmaceutical applications where a discrete value is required without interpretation by an operator.

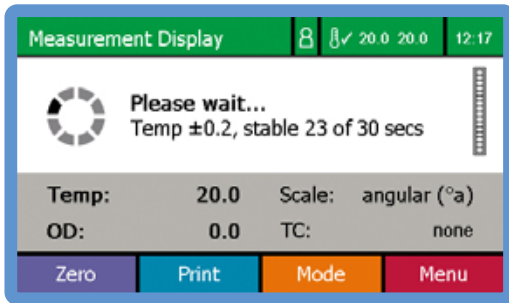


The PHR-MEAN Method, integral to both ADP400 Series polarimeters, allows a number of different readings to be taken from a batch of samples and the statistical report, showing the average, high and low results together with standard deviation can then be printed or stored to file.

The expanded memory ensures that over 8000 measurements and recorded logs of instrument configuration can be saved and viewed or output to LIMS.

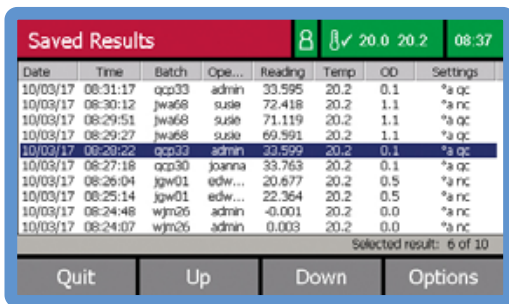

Calibration and configuration can be password protected, accessible by keypad entry or, for convenience, using a fully configurable RFID tag. This, together with the audit trail, facilitates operation in environments conforming to FDA regulation 21 CFR Part 11 or GLP. ADP400 Series polarimeters are also ideal for use within laboratories where compliance with Pharmacopoeia is required.

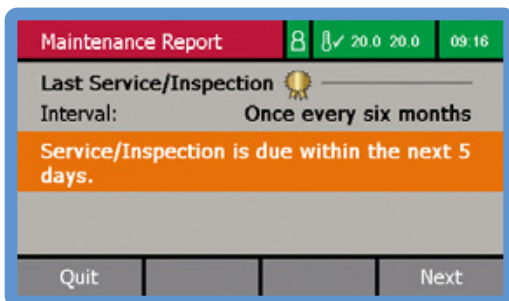

The ADP400 Series polarimeters incorporate a number of industry standard interfaces making it easy to connect to peripheral devices including barcode readers, printers and USB memory sticks for external storage. With the addition of a USB memory stick operators can output results to a secure PDF using the "Print to Secure PDF." The USB port can also be used to accept RS232 via an available adaptor.

There are two instruments in the ADP400 Series.



ADP430 Polarimeter

The ADP430 is a fully featured instrument designed for use in applications where internal temperature control is not required or where the use of automatic temperature compensation or a water bath is preferred, such as within the food industry.

ADP450 Polarimeter


The ADP450 polarimeter with patented XPC technology features interchangeable contact Peltier plates facilitating measurement at a stable temperature using Peltier control. XPC technology conveniently stabilises the temperature of the sample being measured. With SMART temperature stability enabled, the ADP450 will only give a result when the instrument has displayed a stable temperature over a predetermined timeframe, making for reliable results in compliance with good laboratory practice.



- Peltier or waterbath
- Continuous or single read
- Three decimal places
- PHR-MEAN Method
- Conforms to USP/EP/BP
- Standard sample tubes

XPC Technology

- Fill the tube
- Slot the tube in to the XPC adaptor
- Place in to the ADP450
- Wait for SMART stability
- Record the reading

| Temperature | ADP430 | ADP450 (Peltier) |  |
|------------------|--------------------------------------|-------------------------|-------------------------------------------------------------------------------------|
| Order Code | 37-30 | 37-50 | |
| Control | None or external waterbath | Patented XPC Technology | |
| Compensation | None, ICUMSA, Quartz or User Defined | | |
| Measuring Range | 5-40 °C | 15-35 °C | |
| Sensor Accuracy | ± 0.1 °C | ± 0.1 °C | |
| Stability | Waterbath dependent | ± 0.2 °C | |
| Stability Checks | None/delay on single-shot | None/delay or SMART | |

Polarimeter Tube - Spare Parts

| Code | Description | Diameter ¹ | Quantity | Tube Type |
|-------|--------------------------------------------------------|-----------------------|----------|-----------|
| 35-60 | Low strain cover glasses | 15.5 | 12 | Glass |
| 35-64 | Rubber washers for use between cover glass and end cap | 15.5 | 122 | |
| 35-68 | End caps, plastic | 15.5 | | |
| 35-20 | End caps, metal | 15.5 | 2 | Glass |
| 35-21 | Rubber Glands for metal end cap tubes & fitting tool | 15.5 | 12 | |
| 35-62 | Low strain cover glasses | 22.5 | 2 | Flow |
| 35-66 | Rubber washers for use between cover glass and end cap | 22.5 | 2 | |
| 35-88 | End Caps, stainless steel | 22.5 | 2 | |
| 35-79 | Temperature sensor saddle | - | 1 | Low |
| 35-80 | Low strain cover glasses | 20 | 6 | Volume |
| 35-81 | Rubber washers for use between cover glass and end cap | 20 | 10 | |

Polarimeter Tubes

Bellingham + Stanley polarimeter tubes are manufactured to high quality standards conforming to ICUMSA recommendations and are compatible with most makes of polarimeter.

Tube ends are precision ground with windows made from specially selected low strain glass in order to achieve highest accuracy optical rotation measurement.

Special tubes, XPC adaptors and cover glasses for ultra-violet measurement are also available. Please visit our website for further details.



| Code | Standard Glass - 8mm | Length | Fig. |
|-------|-----------------------------------------------------------------------------|----------|------|
| 35-29 | Bubble type - to clear bubble from field of view Most suited to Model D7 | 100 | 1 |
| 35-30 | | 200 | |
| 35-28 | | 50 - 200 | |
| 35-46 | Centre fill - for easy filling and placement of ADP temperature sensor | 100 | 2 |
| 35-47 | | 200 | |
| 35-45 | | 50 - 200 | |
| 35-57 | Cup - funnel shaped centre fill for viscous samples | 100 | 3 |
| 35-58 | | 200 | |
| 35-56 | | 50 - 200 | |
| 35-10 | Metal end - centre fill for aggressive chemicals and solvents | 100 | 4 |
| 35-11 | | 200 | |

Volume: 5.02ml/100mm.

| Code | Flow & Temperature Control - 8mm | Lid code | Length | Fig. |
|-------|----------------------------------|----------|--------|------|
| 36-57 | Funnel flow-through tube | 37-012 | 100 | 5 |
| 36-58 | | 37-011 | 200 | |
| 36-67 | Continuous flow-through tube | 37-012 | 100 | 6 |
| 36-68 | | 37-011 | 200 | |
| 36-77 | Centre fill tube | 37-010 | 100 | 7 |
| 36-78 | | 37-009 | 200 | |

| Code | Low Volume - Leur - 5mm | Volume | Lid/Fig. |
|-------|-----------------------------|--------|------------------|
| 35-71 | 50mm stainless steel tube | 1.0 | 37-010 Fig. 8 |
| 35-72 | 25mm stainless steel tube | 0.5 | |
| 35-73 | 10mm stainless steel tube | 0.2 | |
| 35-74 | 5mm stainless steel tube | 0.1 | |
| 35-78 | 50mm glass loaded PTFE tube | 1.0 | |
| 35-77 | 25mm glass loaded PTFE tube | 0.5 | |

All lengths in millimetres. Volumes in millilitres. All collar sizes 30mm diameter. For use with ADP/S models, polarimeter tubes figure 5 to 8 require slotted lids.

ADP600 Polarimeters



Available as single, dual and multiple wavelength derivatives not only covering the visible spectrum, the new ADP600 Series of Peltier temperature controlled polarimeters are capable of measuring optical rotation to four decimal places in the highly sensitive ultra-violet region. This capability makes the instrument particularly suited for use by scientists wishing to measure chiral compounds and other optically active substances in the chemical, pharmaceutical and food sectors as well as for use in academic research.

Technology is intelligently applied to the sample new polarimeters so that measurement can be without the need of an external waterbath.

The ADP600 Series Polarimeters have two preset operating temperatures being 20 and 25 °C in accordance with European and United States Pharmacopoeia respectively and other user temperatures between 20 and 30°C may be configured via the instrument user interface.

ADP600 Series Polarimeters accept standard glass or special low volume leur taper polarimeter tubes facilitating measurement across optical path lengths between 5 and 200m with tube diameters from 3 to 8mm being readable. Optional lids may be easily be fitted to the ADP600 Series Polarimeters, facilitating sample tube entry and exit.

Integral to operational simplicity is the full colour, high definition, touch-screen graphical user interface. A menu structure featuring

Specifications

| | |
|--------------------------------|-----------------------------------------------------------------------|
| Range (°A) | ± 89 (-355 to +355 via Method selection) |
| Resolution (°A) | 0,0001 |
| Accuracy (°A) | ± 0.003 (@546 & 589 nm) / ± 0.005 (@325, 365, 405 & 436 nm) |
| Temperature Range | 15-35°C |
| Temperature Control / Accuracy | Peltier / ± 0.2°C |
| Temperature Compensation | None, sugar, quartz, user defined |
| Optical Density Range | 0.0 a 3.0 OD |
| Methods | Specific Rotation, % Concentration, % Invert Sugar, % Inversion (A-B) |
| Temperature Set Points | 20 & 25 °C (variable between 20-30 °C via Method) |
| Reading Time | 15-60 seconds @ 546/589nm and 20/20°C (instrument/sample) |
| Tube Length | 5-200 mm |
| Tube Diameter | 3-8 mm |
| User Interface | High Definition 7.4" touch-screen colour display |
| Light Source | UV/Vis lamp (6V, 2A >1000hrs) and narrow band pass filter(s) |
| Interfaces | 3 x USB (A), 1 x USB (B), 1 x Ethernet, 1 x Serial (RS232) |
| Power Supply | 100-250V~, 50-60 Hz. <6A. |




a METHODS system makes for one-touch calibration and instrument configuration; especially where the specific rotation of a number of samples is being analysed over a wide range of concentrations, path lengths, temperatures and wavelengths. A “Mean Method” is also available, allowing a number of readings to be taken from a production batch with the mean being calculated and recorded once the experiment has been completed.

- Simple Methods system
- Accepts standard & low volume sample tubes
- Supports FDA regulation 21 CFR Part 11
- US/EP/JP compliant

ADP600 Series Polarimeters have an extensive interfacing capability. Four USB ports provide excellent connectivity to, for example, convenient remote keyboards, printers, barcode readers and LIMS or PC, whilst the Ethernet connection may be used for networking as well as remote diagnostics or certification. The ADP600 Series on-board RFID reader may be used to identify users as well as sample tube lengths for recording and in particular, calculation of Specific Rotation.

Additionally the ADP600 Series Polarimeters feature a secure “print to PDF” function that may be configured to operate in secure environments in accordance with FDA regulation 21 CFR Part 11 and importantly, the ADP600 Series polarimeters meet all of the requirements, including wavelength directives of British, United States, European and Japanese Pharmacopoeia.

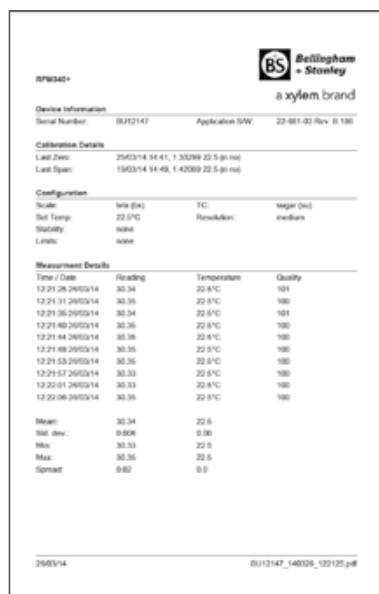

| Code | Description | Wavelengths(s) |
|-------|----------------------------------------|----------------------------------|
| 37-61 | ADP610 single wavelength polarimeter | 589 nm |
| 37-62 | ADP620 dual wavelength polarimeter | 546 & 589 nm |
| 37-63 | ADP622 dual wavelength polarimeter | 365 & 589 nm |
| 37-64 | ADP640 multiple wavelength polarimeter | 405, 436, 546 & 589 nm |
| 37-65 | ADP650 multiple wavelength polarimeter | 365, 405, 436, 546 & 589 nm |
| 37-66 | ADP660 multiple wavelength polarimeter | 325, 365, 405, 436, 546 & 589 nm |

ADS400 Series Saccharimeter

The ADS400 Series Saccharimeter is a purpose built polarimeter that displays results in the ISS (°Z) scale.

This series of Bellingham + Stanley instruments has been primarily designed for busy sugar laboratories, factories and tare houses. The ADS400 Series is available in 2 wavelengths: Sodium (589nm) and NIR (850nm), which facilitates "lead-free measurement". Both models can be purchased with or without XPC Technology - Xylem's patented Peltier temperature control system.



The ADS400 Series Saccharimeters are designed to operate in isolation but work best when connected to an RFM Refractometer to create a complete Purity system that facilitates accurate purity readings.

The ADS400 Series is built in the UK using a corrosion-free polyurethane foam case - sealed to prevent moisture and dust ingress to its optics. Low power consumption and low maintenance is achieved using an LED light source which offers light for the length of the product lifetime¹.

The external power unit keeps internal temperatures minimal and in combination with the sealed casing makes the ADS400 Series Saccharimeter a great choice for working in high humidity environments.

Thanks to its intelligent setup wizard, easy-to-use keypad with colourful HD display and intuitive software, operating the ADS400 Series is quick and simple. RFID login allows several levels of access, as well as offering an audit trail, meaning settings can be hidden away so users can only take readings; ideal for allowing use of the instrument no matter what level of training.

A METHODS system allows for quick configuration, with reading type (continuous or single-shot) and limit checking against pre-defined product specifications made simple. Configurable Purity equations are also accessible through the easy-to-use software using the keypad.

¹ LED lifetime guaranteed through normal use and with no interference.

Measurement Display 8 20.0 20.0 09:21

purity **99.06** °z: 99.34
Brix: 25.89

Temp: 20.0 Scale: purity
OD: 0.1 TC: sugar
Tube Len: 200mm

Zero Save Mode Menu

Equation 8 20.0 20.0 13:49

User Defined:

Note _____
See user guide for information.

Quit Backspace Enter

Saved Results 8 20.0 20.2 08:37

| Date | Time | Batch | Op... | Reading | Temp | OD | Settings |
|----------|----------|-------|--------|---------|------|-----|----------|
| 10/03/17 | 08:31:17 | qcp33 | admin | 33.595 | 20.2 | 0.1 | *a qc |
| 10/03/17 | 08:30:12 | jwa68 | suse | 72.418 | 20.2 | 1.1 | *a nc |
| 10/03/17 | 08:29:51 | jwa68 | suse | 71.119 | 20.2 | 1.1 | *a qc |
| 10/03/17 | 08:29:27 | jwa68 | suse | 69.591 | 20.2 | 1.1 | *a qc |
| 10/03/17 | 08:28:22 | qcp33 | admin | 33.599 | 20.2 | 0.1 | *a qc |
| 10/03/17 | 08:27:18 | qcp30 | joanna | 33.763 | 20.2 | 0.1 | *a qc |
| 10/03/17 | 08:26:04 | ggw01 | edw... | 20.677 | 20.2 | 0.5 | *a nc |
| 10/03/17 | 08:25:14 | ggw01 | edw... | 22.364 | 20.2 | 0.5 | *a nc |
| 10/03/17 | 08:24:48 | wym06 | admin | -0.001 | 20.2 | 0.0 | *a nc |
| 10/03/17 | 08:24:07 | wym06 | admin | 0.003 | 20.2 | 0.0 | *a nc |

Selected result: 6 of 10

Quit Up Down Options



- ATC or Patented XPC Peltier
- ICUMSA and Tropical Scale ATC
- Funnel flow or standard tube packages
- High definition 4" full colour display
- Continuous or single shot readings

Latest Software Features

- Save over 8000 readings
- Methods system with limits
- Connectable to refractometer
- Onboard Purity
- User audit trail
- Date/Time for GLP
- USB "Back-up & Clone"
- User maintenance prompts

| General Specifications | Sodium (589nm) | NIR (850nm) |
|--------------------------------|------------------------------------------|-------------------------|
| Scales | | |
| International Sugar Scale (°Z) | -225 a +225 | -225 a +225 |
| User Scales/Methods | 100 | 100 |
| Resolution | | |
| International Sugar Scale (°Z) | 0.01/0.001 (selectable) | 0.01/0.001 (selectable) |
| Accuracy | | |
| International Sugar Scale (°Z) | ± 0.030 | ± 0.060 |
| Precision (Reproducibility) | | |
| International Sugar Scale (°Z) | ± 0.005 | ± 0.010 |
| Interfaces | 1 x USB (A), 1 x USB (B), 1 x Ethernet | |
| Data Output | Print to USB, print to printer, csv, XML | |

| Temperature Specifications | ADS400 ATC | ADS400 XPC (Peltier) |
|----------------------------|------------------------------------------------|-------------------------|
| Compensation | None, ICUMSA, Tropical, Quartz or User Defined | |
| Control | None or external waterbath | Patented XPC Technology |
| Measuring Range | 5-40 °C | 15-35 °C |
| Sensor Accuracy | ± 0.1 °C | ± 0.1 °C |
| Stability | Waterbath dependent | ± 0.2 °C |
| Stability Checks | None/delay on single-shot | None/delay or SMART |

The ADS400 Series Saccharimeter is available in predefined packages to make choosing the right system as simple as possible. All packages are supplied with appropriate cell, lid, onboard purity, LIMS logger PC software, RFID tags & certificate of conformity.

| | ADS400 ATC | | | ADS400 XPC (Peltier) | | |
|---------------|-------------|--------------|--------------|----------------------|--------------|--------------|
| | 200mm Glass | 100mm Funnel | 200mm Funnel | 200mm Metal | 100mm Funnel | 200mm Funnel |
| Sodium | ADS435 | ADS435-F100 | ADS435-F200 | ADS455 | ADS455-F100 | ADS455-F200 |
| (order code) | 37-25 | 37-26 | 37-27 | 37-45 | 37-46 | 37-47 |
| NIR | ADS438 | ADS438-F100 | ADS438-F200 | ADS458 | ADS458-F100 | ADS458-F200 |
| (order code) | 37-85 | 37-86 | 37-87 | 37-95 | 37-96 | 37-97 |

Certified Reference Materials

Regular verification of laboratory instrumentation is of primary importance in a modern manufacturing facility, not only for reasons of quality control but also as an assurance of plant efficiency.

Depending on the instrument type, application and traceability requirement, a choice can be made from a number of Certified Reference Materials offered by Bellingham + Stanley that may be used to verify almost any make of refractometer or polarimeter. All CRMs are manufactured to the highest standards and are certified in accordance with ISO/IEC 17025:2017.



AG Fluids

Ideal for use where verification/calibration at the lower end of the °Brix or refractive index scale is required. AG fluids are despatched with at least 12-months validity and when purchased as a 'multi-pack' offer excellent value for money as the 'per bottle shipping cost' is significantly reduced.

Calibration Oils

Primarily used to verify instruments that operate over a wide refractive index range and for specific applications such as within the edible oil industry, careful consideration to temperature must be adopted when using calibration oils due to their high coefficient. For optimum performance, temperature control should be applied to the instrument being verified or alternatively, use of the RI/°C table/calculator should be made.



Specification

| | |
|---------------|---------------------------------|
| Certificate: | UKAS (ISO 17025) |
| Shelf Life: | 12-months (minimum) |
| Storage: | Room temperature Keep sealed |
| Traceability: | ICUMSA / NIST |

Uncertainty

| | RI | °Brix |
|--------------------|------------|---------|
| AG2.5-40 | ± 0.000037 | ± 0.019 |
| Oil BSLP/ BSDCB | ± 0.000074 | ± 0.030 |
| Oil BSDD | ± 0.000103 | -- |

| Code | | Specification | |
|------------|----------------------------------|------------------------|----------------------|
| Type | Multi-pack of 5 x 5ml Bottles | Refractive Index | °Brix |
| AG2.5 | 90-501 | 1.33659 | 2.50 |
| AG5 | 90-502 | 1.34026 | 5.00 |
| AG7.5 | 90-503 | 1.34401 | 7.50 |
| AG10 | 90-504 | 1.34782 | 10.00 |
| AG11.2 | 90-505 | 1.34968 | 11.20 |
| AG12 | 90-506 | 1.35093 | 12.00 |
| AG12.5 | 90-507 | 1.35171 | 12.50 |
| AG15 | 90-508 | 1.35568 | 15.00 |
| AG-AUS | 90-521 | 1.38290 | 30.98 |
| AG40 | 90-518 | 1.39986 | 40.00 |
| Oil BSLP | 90-525 | 1.46990 ^{2/4} | 71.81 ^{3/4} |
| Oil BSDC-B | 90-531 | 1.53632 ^{2/4} | 96.61 ^{3/4} |
| Oil BSDD | 90-535 | 1.56138 ^{2/4} | -- |

The United Kingdom Accreditation Service (UKAS) is one of the signatories to the International Laboratory Accreditation Co-operation (ILAC) Arrangement for the mutual recognition of calibration certificates.

Please contact Bellingham + Stanley or your local distributor for advice on selecting the correct CRM for your particular application.

Note:

- UKAS Certification is valid at 20°C & 589.3nm only. For use at other temperatures, please refer to the calibration/technical sections of www.bellinghamandstanley.com
- Typical refractive index @ 589.3nm & 20.0°C.
- Equivalent °Brix value @ 589.3nm & 20.0°C. °Brix values greater than 85 are extrapolated from the relationship given in ICUMSA SPS-3 (2000) Equation 2.
- All quoted values for calibration oils are subject to minor batch to batch variations.

Sucrose Solutions

Sucrose Solutions are an extremely easy to use medium for verifying and calibrating refractometers measuring in the °Brix scale, as no special consideration is required when testing instruments at ambient temperature fitted with ATC.

Sucrose Solutions are typically supplied in 15ml plastic dropper bottles complete with Certificate of Calibration but may also be supplied in a larger quantity for high volume users or for customers wishing to verify the performance of density meters operating in the °Brix scale.

The Certificate of Calibration provides values for sucrose in %weight/weight, °Brix and refractive index as well as giving detail about traceability and uncertainty.

Sucrose Solutions - Supply Contracts

As sucrose solutions have a limited shelf life of 6-weeks, they must be purchased at the time of requirement. If a frequent calibration regime is operated, the administration cost of issuing purchase orders every time can be relatively high. Many users therefore choose to take out a supply contract on a single order that ensures trouble free regular delivery over a twelve month period.



| Code | Value (°Brix) | Value (RI) |
|-------|---------------|------------|
| SS00 | 0 | 1.33299 |
| SS05 | 5 | 1.34026 |
| SS075 | 7.5 | 1.34401 |
| SS10 | 10 | 1.34782 |
| SS112 | 11.2 | 1.34968 |
| SS115 | 11.5 | 1.35015 |
| SS12 | 12 | 1.35093 |
| SS125 | 12.5 | 1.35171 |
| SS15 | 15 | 1.35568 |
| SS20 | 20 | 1.36384 |
| SS25 | 25 | 1.37233 |
| SS30 | 30 | 1.38115 |
| SS35 | 35 | 1.39032 |
| SS40 | 40 | 1.39986 |
| SS45 | 45 | 1.40978 |
| SS50 | 50 | 1.42009 |
| SS55 | 55 | 1.43080 |
| SS60 | 60 | 1.44193 |

Specification (Sucrose)

| | |
|-------------------|---------------------------------------------|
| Certificate: | Manufacturer |
| Uncertainty (k=2) | ±0.011 °Brix |
| Shelf Life: | 6 weeks |
| Storage: | Refrigerated at approx 5°C Do not freeze |
| Traceability: | ICUMSA / NIST |

| Code | ISS (°Z) | °A | Specification |
|--------|-------------------------------------------------------------------------------------------------------------------------|----------|--------------------------------------------------------------------------------|
| 34-20 | +100 °Z | +34.6 °A | Standard Quartz Control Plate and Certificate of Conformity at 589nm and 850nm |
| 34-21 | +15 °Z | +5.2 °A | |
| 34-22 | -30 °Z | -10.4 °A | |
| 90-803 | UKAS Certificate of Calibration for Quartz Control Plate at 589.44nm | | |
| 90-805 | UKAS Certificate of Calibration for Quartz Control Plate at additional specified wavelength between 546-900nm | | |
| 90-807 | Manufacturer's certificate of calibration for Quartz Control Plate at additional specified wavelength between 300-545nm | | |
| 34-241 | Thermal Block for use with ADP/S | | |



Specification (Quartz Control Plate)

| | |
|-------------------|-------------------|
| Certificate: | UKAS (ISO 17025) |
| Best Measurement | ± 0.017 °Z |
| Uncertainty (k=2) | ± 0.006 °A |
| Shelf Life: | Certify Regularly |
| Traceability: | ICUMSA / PTB |

Accessories

Code Flowcell Accessories

| Code | Flowcell Accessories | RFM300-T/M | RFM900-T |
|-------|-----------------------------------------------------------------------------------------------------------------|------------|----------|
| 19-98 | RFM300 micro flowcell, polyacetyl, UNF 28/nozzle | ✓ | |
| 19-84 | RFM300 macro flowcell, polyacetyl, UNF 28/nozzle | ✓ | |
| 19-85 | RFM300 funnel flowcell, polyacetyl, UNF 28/nozzle, 100mm (diameter) stainless steel funnel and anti-syphon tube | ✓ | |
| 19-91 | RFM900 micro flowcell, PEEK, UNF 28/nozzle | | ✓ |
| 19-92 | RFM900 macro flowcell, PEEK, UNF 28/nozzle | | ✓ |
| 75-60 | Material Certificate for wetted components | | ✓ |



Code Peripherals & Cables

| Code | Peripherals & Cables | RFM700-M | RFM-T/M | ADP400 | ADP600 |
|--------|--------------------------------------------------------|----------|---------|--------|--------|
| 55-14 | CBM-910 Dot Matrix Printer - Serial: UK/Euro Plug 220V | ✓ | ✓ | ✓ | ✓ |
| 55-16 | CBM-910 Dot Matrix Printer - Serial: USA Plug 110V | ✓ | ✓ | ✓ | ✓ |
| 55-18 | Thermal printer USB: 110-240V, 50/60Hz | ✓ | ✓ | ✓ | ✓ |
| 54-02 | Serial Cable for CBM910 Serial printer | ✓ | ✓ | ✓ | ✓ |
| 55-85 | USB to RS232 Adaptor | ✓ | ✓ | ✓ | ✓ |
| 55-075 | LAN cable male/male (2m) | | ✓ | ✓ | ✓ |
| 55-081 | USB Cable A to A male/male (2m) | ✓ | ✓ | ✓ | ✓ |
| 55-082 | USB Cable A to B male/male (2m) | ✓ | ✓ | ✓ | ✓ |
| 55-82 | Barcode Reader - USB | ✓ | ✓ | ✓ | ✓ |
| 55-86 | USB Mini Keyboard | ✓ | ✓ | ✓ | ✓ |
| 55-88 | USB Hub | ✓ | ✓ | ✓ | ✓ |



Code Spare Parts

| Code | Spare Parts | RFM700-M | RFM-T/M | ADP400 | ADP600 |
|--------|-------------------------------------------------|----------|---------|--------|--------|
| 19-98 | Contact Presser for Viscous Samples (from 2019) | ✓ | ✓ | | |
| 19-201 | RFM-T/M Spare Filter (12 pk) | | ✓ | | |
| 19-204 | Touchscreen Protector | | ✓ | | ✓ |
| 19-203 | Touchscreen Stylus | | ✓ | | ✓ |
| 22-071 | RFID tags (3 pk) | ✓ | ✓ | ✓ | |
| 22-072 | RFID tags (10 pk) | ✓ | ✓ | ✓ | |
| 55-250 | Waterproof Power Supply (IP65) | ✓ | ✓ | ✓ | |



Features Guide

Refractometers

| | RFM700-M | RFM300-T/M | RFM900-T |
|-------------------------------------------------------------|----------|------------|----------|
| Brix / Refractive Index / User Scales | ✓ | ✓ | ✓ |
| Dual Scale Display Function | ✓ | ✓ | |
| Equivalent SG Scale for Beverage | ✓ | | |
| High RI Range | | | ✓ |
| Peltier Temperature Control | ✓ | ✓ | |
| Delay Before Reading | ✓ | ✓ | ✓ |
| SMART Temperature Stability | ✓ | ✓ | |
| Presser | ✓ | ✓ | |
| Continuous / Auto-read | ✓ | ✓ | ✓ |
| Zero Calibration at any value < Span | ✓ | ✓ | |
| Calibration & Configuration Audit Trail | ✓ | ✓ | |
| On-board Multi-lingual Menu Structure | ✓ | ✓ | ✓ |
| Installation Wizard | ✓ | ✓ | ✓ |
| Security (Password) | ✓ | ✓ | ✓ |
| Facilitates 21 CFR Part 11 | ✓ | ✓ | |
| RFID User Clearance | ✓ | ✓ | |
| Store Data (8000 results) | ✓ | ✓ | ✓ |
| View Data | ✓ | ✓ | |
| Output Data | ✓ | ✓ | ✓ |
| GLP Printout (Date/Time) | ✓ | ✓ | ✓ |
| CSV Data String for LIMS/Print PDF | ✓ | ✓ | ✓ |
| Methods System | ✓ | ✓ | |
| Mean Method (USP/EP/BP) | ✓ | ✓ | |
| Petroleum Method ASTM D 2140, 1218, 1747, 5006 | | | ✓ |
| Coffee Method | ✓ | ✓ | |
| Beverage Method Citric Acid Correction, Apparent Brix/SG | | ✓ | |
| Flow Cell Option | OPT | OPT | |
| Hi Accuracy "Urea" option | | | ✓ |
| Remote PC Software | ✓ | ✓ | ✓ |

Polarimeters

| | ADS400 | ADP430 | ADP450 | ADP600 |
|-----------------------------------------|--------|--------|--------|--------|
| Single Wavelength | ✓ | ✓ | ✓ | ✓ |
| Multiple Wavelength | | ✓ | | |
| Peltier Temperature Control | | ✓ | ✓ | |
| Smart Temperature Stability | ✓ | ✓ | | |
| Angular (°A) | ✓ | ✓ | ✓ | |
| ISS (°Z) | ✓ | ✓ | ✓ | |
| Range Configuration (-355 to +355°A) | ✓ | ✓ | ✓ | |
| Optical Density Display | ✓ | ✓ | ✓ | |
| ATC (Sugar/Quartz/None) | ✓ | ✓ | ✓ | ✓ |
| Zero & Span Calibration | ✓ | ✓ | ✓ | ✓ |
| Calibration & Configuration Audit Trail | ✓ | ✓ | ✓ | |
| Touch-screen Display | | ✓ | | |
| On-board Multi-lingual Menu Structure | ✓ | ✓ | ✓ | |
| Security (password) | ✓ | ✓ | ✓ | |
| Facilitates 21 CFR 11 | ✓ | ✓ | ✓ | |
| RFID User | ✓ | ✓ | ✓ | |
| Reading Log (8000 results) | ✓ | ✓ | ✓ | |
| GLP Printout (Date/Time/Batch) | ✓ | ✓ | ✓ | |
| CSV Data String for LIMS | ✓ | ✓ | ✓ | ✓ |
| Print to Secure PDF | ✓ | ✓ | ✓ | |
| NIR Wavelength | OPT | | | |
| High OD Performance | ✓ | ✓ | ✓ | |
| Methods System | ✓ | ✓ | ✓ | |
| Mean Method (USP/EP/BP) | ✓ | ✓ | ✓ | |
| Specific Rotation Method | ✓ | ✓ | ✓ | |
| Concentration Method | ✓ | ✓ | ✓ | |
| % Inversion (Sucrose) or Invert Sugar | ✓ | ✓ | ✓ | |
| USB Connectivity | ✓ | ✓ | ✓ | |
| Flow Package Options | ✓ | OPT | OPT | OPT |
| Low Volume Cell Options | ✓ | OPT | OPT | OPT |
| PC /LIMS Logger | ✓ | ✓ | ✓ | ✓ |

OPT - optional extra at time of purchase.

Xylem |'zīləm|

- 1) The tissue in plants that brings water upward from the roots;
- 2) a leading global water technology company.

Bellingham + Stanley is part of Xylem Analytics and a leading provider of refractometers and polarimeters.

Xylem Analytics' global brands have been leaders in the laboratory instrumentation market for decades, and are relied upon every day across more than 150 countries. Working in true partnership with our clients, we listen, learn and adapt to individual needs, offering deep application expertise built upon our long history of innovation in instruments and services. Our solutions for analysis, measurement and monitoring help enable many of today's modern laboratories and industrial processes, and provide our customers the trusted and high performing solutions they need to succeed.

Xylem Analytics is part of Xylem Inc., a global company focused on solving the world's most challenging and fundamental water issues. As accurate analysis is crucial to the water industry, Xylem Analytics taps its diverse product brands for leadership in that field and beyond, providing the best laboratory and field monitoring instrumentation across a wide variety of industries.

For more information on how Xylem can help you, go to www.xylem.com



Bellingham + Stanley

Xylem
Longfield Road
Tunbridge Wells
Kent, TN2 3EY
United Kingdom

Tel: +44 (0) 1892 500400

Email: sales.bs.uk@xyleminc.com
www.bellinghamandstanley.com

Bellingham + Stanley (USA)

Xylem
1700/1725 Brannum Lane
Yellow Springs
OH 45387

Tel: +1 (937) 688 4255
USA: +1 (877) 726 0975

Email: sales.bs.us@xyleminc.com